



Boston Electronics Corporation

91 Boylston Street, Brookline MA 02445 USA
(800)347-5445 or (617)566-3821 fax (617)731-0935

www.boselec.com

tcspc@boselec.com

What is Time Correlated Single Photon Counting?

Introduction to
The Becker & Hickl
SPC-series Module Family

PC Based
Systems



Becker & Hickl GmbH
Kolonnenstrasse 29
10829 Berlin, Germany
Tel. +49 30 787 56 32
Fax. +49 30 787 57 34
www.becker-hickl.de
info@becker-hickl.de

TCSPC1.DOC

Time-Correlated Single Photon Counting

Time-Correlated Single Photon Counting (TCSPC) is a technique to record low level light signals with picosecond time resolution. Typical applications are

- Ultra-Fast Recording of Optical Waveforms**
- Fluorescence Lifetime Measurements**
- Detection and Identification of Single Molecules**
- DNA Sequencing**
- Optical Tomography**
- Fluorescence Lifetime Imaging**

The method has some striking benefits:


- Ultra-High Time Resolution - 25 ps fwhm with the best detectors**
- Ultra-High Sensitivity - down to the Single Photon Level**
- Short Measurement Times**
- High Dynamic Range - Limited by Photon Statistics only**
- High Linearity**
- Excellent Signal-to-Noise Ratio**
- High Gain Stability**
- Suppression of Detector Leakage Currents**

TCSPC works best for

- High Repetition Rate Signals (MHz Range)**
- Wavelengths from 160 nm to 1000 nm**

Measurement Principle

Time-Correlated Single Photon Counting is based on the detection of single photons of a periodical light signal, the measurement of the detection times of the individual photons and the reconstruction of the waveform from the individual time measurements. The method makes use of the fact that for low level, high repetition rate signals the light intensity is usually so low that the probability of detecting one photon in one signal period is much less than one. Therefore, the detection of several photons can be neglected and the principle shown in the figure below can be used:

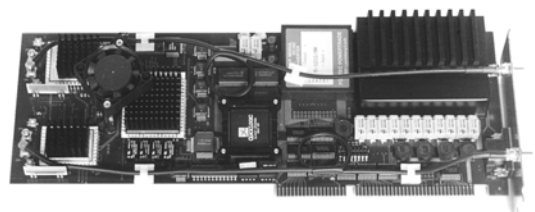

Complete electronics on board - a TCSPC Module of Becker & Hickl

The detector signal consists of a train of randomly distributed pulses due to the detection of the individual photons. There are many signal periods without photons, other signal periods contain one photon pulse. Periods with more than one photon are very rare.

When a photon is detected, the time of the corresponding detector pulse is measured. The events are collected in memory by adding a '1' in a memory location with an address proportional to the detection time. After many photons the histogram of the detection times, i.e. the waveform of the optical pulse, builds up in the memory.

Although this principle looks complicated at the first glimpse, it is very efficient and accurate for the following reasons:

The accuracy of the time measurement is not limited by the width of the detector pulse. Thus, the time resolution is much better than with the same detector used in front of an oscilloscope or another linear signal acquisition device. Furthermore, all detected photons contribute to the result of the measurement. There is no loss due to 'gating' as in 'Boxcar' devices or gated image intensified CCDs.

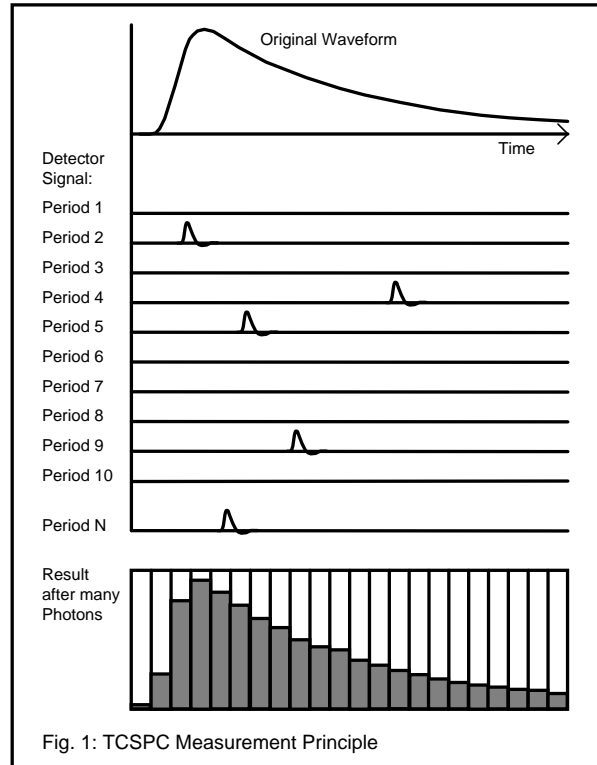


Fig. 1: TCSPC Measurement Principle

Sensitivity

The sensitivity of the SPC method is limited mainly by the dark count rate of the detector. Defining the sensitivity as the intensity at which the signal is equal to the noise of the dark signal the following equation applies:

$$S = \frac{(R_d * N/T)^{1/2}}{Q}$$

(R_d = dark count rate, N = number of time channels, Q = quantum efficiency of the detector, T = overall measurement time)

Typical values (uncooled PMT with multialkali cathode) are $R_d=300s^{-1}$, $N=256$, $Q=0.1$ and $T=100s$. This yields a sensitivity of $S=280$ photons/second. This value is by a factor of 10^{15} smaller than the intensity of a typical laser (10^{18} photons/second). Thus, when a sample is excited by the laser and the emitted light is measured, the emission is still detectable for a conversion efficiency of 10^{-15} .

Time resolution

The SPC method differs from methods with analog signal processing in that the time resolution is not limited by the width of the detector impulse response. For the SPC method only the timing accuracy in the detection channel is essential. This accuracy is determined by the transit time

spread of the single photon pulses in the detector and the trigger accuracy in the electronic system. The timing accuracy can be up to 10 times better than the half width of the detector impulse response. Some typical values for different detector types are given below.

Conventional photomultipliers

standard types 0.6 ... 1 ns

high speed (XP2020) 0.35 ns


Hamamatsu TO8 photomultipliers

R5600, R5783 140 ... 220 ps

microchannel plate photomultipliers

Hamamatsu R3809 25 ... 30 ps


avalanche photodiodes 60 ... 500 ps

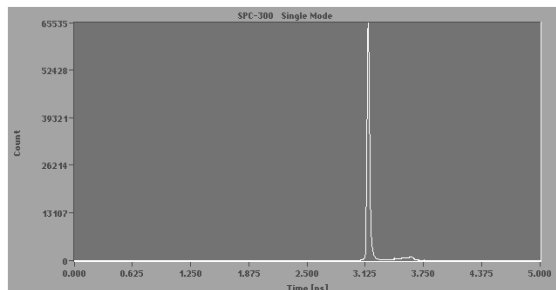

A laser pulse recorded with 30 ps fwhm

Accuracy


The accuracy of the measurement is given by the standard deviation of the number of collected photons in a particular time channel. For a given number of photons N the signal-to-noise ratio is $SNR = N^{1/2}$. If the light intensity is not too high, nearly all detected photons contribute to the result. Therefore, the SPC yields a very good signal-to-noise ratio at a given intensity and measurement time. Furthermore, in the SPC method, noise due leakage currents, gain instabilities, and the stochastic gain mechanism of the detector does not appear in the result. This yields an additional SNR improvement compared to analog signal processing methods.

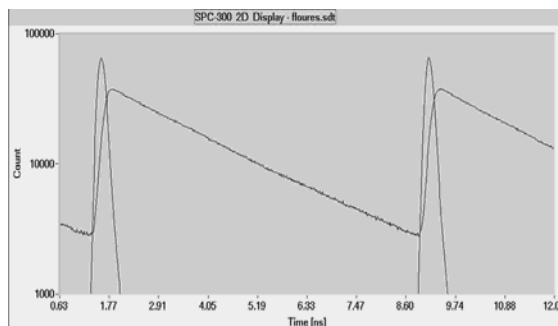

Fluorescence decay curves, excitation with Ar+ laser

Recording Speed

The TCSPC method is often thought to suffer from slow recording speed and long measurement times. This bad reputation comes from traditional TCSPC devices built up from nuclear instrumentation modules which had a maximum count rate of some 10^4 photons per second. State-of-the-art TCSPC devices from Becker & Hickl achieve count rates of some 10^6 photons per seconds. Thus, 1000 photons can be collected in less than 1 millisecond, and the devices can be used for such high speed applications as the detection of single molecules flowing through a capillary, for fast image scanning, for the investigation of unstable samples or simply as optical oscilloscopes.

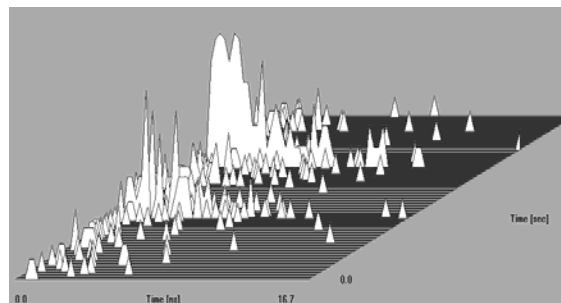

Fluorescence decay signals from single molecules running through a capillary. Collection time 1 ms per curve.

Agents: Boston Electronics Corporation, 91 Boylston Street, Brookline MA 02445

(800)347-5445 or (617)566-3821 * fax (617)7310935 * tcspc@boselec.com * www.boselec.com


B&H What is Time Correlated Single Photon Counting REV 8-08.doc

08/29/08 3:54 PM 4 of 6


Multichannel and Multidetector Capability

Becker & Hickl has introduced multichannel and multidetector capabilities in their TCSPC modules. In the device memory space is provided for several waveforms, and the destination of each individual photon is controlled by an external signal. In conjunction with a fast scanning device, time resolved images are obtained with up to 128 x 128 pixels containing a complete waveform each.

Furthermore, several detectors can be used with one TCSPC module. This technique makes use of the fact that the simultaneous detection of several photons in different detectors is very unlikely. Thus, the output pulses of several detectors are combined and an external 'Routing' device determines in which detector a particular photon was detected. This information is used to route the photons into different memory blocks containing the waveforms for the individual detectors.

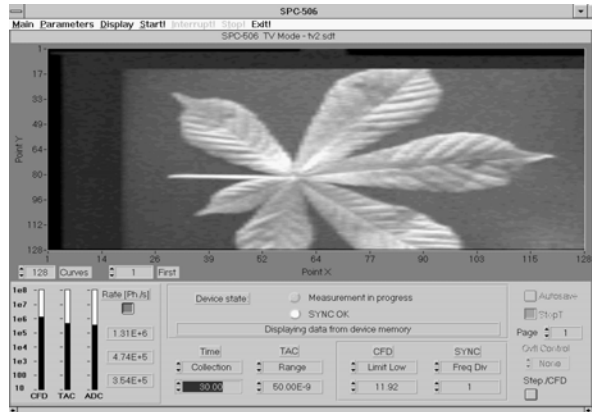


A 128 x 128 pixel scan containing 16384 waveforms

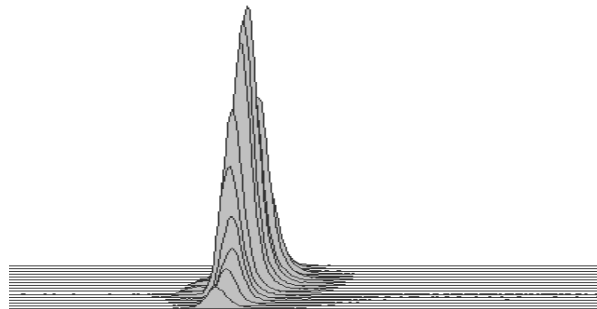

16 signals measured simultaneously with a 16 channel PMT

Return by fax or postal mail or scanned email to the address below



Boston Electronics Corporation


91 Boylston Street, Brookline, Massachusetts 02445 USA
(800)347-5445 or (617)566-3821 fax (617)731-0935
www.boselec.com tcspec@boselec.com

Can we send you a *FREE* bound copy of The bh TCSPC Handbook?

3rd Edition, 466 pages, 503 References
by Wolfgang Becker

For your copy, tell us something about your interest in TCSPC and give us your name and address below so that we can send it to you.

- I am a TCSPC user now
- I am thinking about using TCSPC in the future
- My interest is microscopy
- My interest is single molecule detection
- My interest is _____

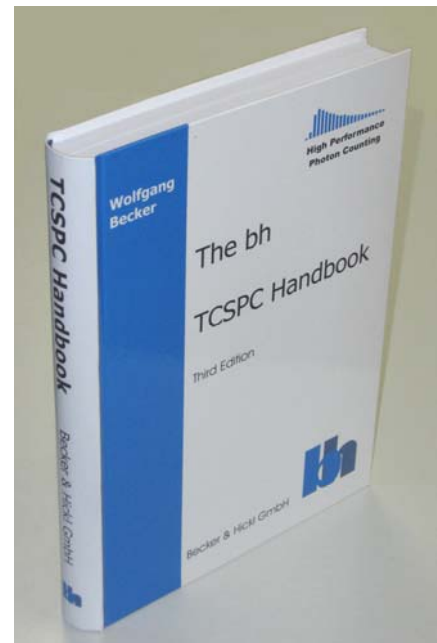

Name: _____

Company or Institution: _____

Address: _____

Also available useful publications (check the box to request):

- TCSPC for Microscopy
- TCSPC Systems
- Photon Counting Detectors for TCSPC
- Picosecond Lasers for TCSPC